




家用血糖機及試紙

Home-use Blood Glucose Meter and Test Strips

購買已於「醫療器械行政管理制度」表列的器械*

Purchase device listed under Medical Device Administrative Control System (MDACS)*

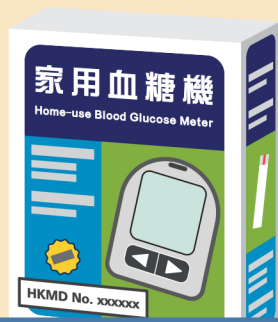


細閱及遵從使用說明

Carefully read and follow the Instruction for Use (IFU)



記錄測試結果

Record test results

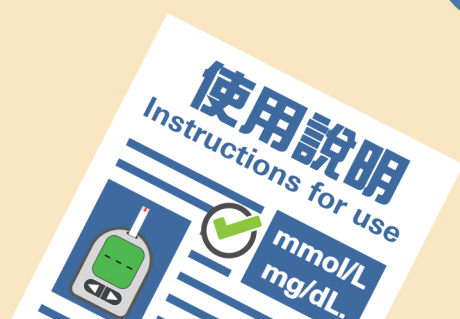


定時按使用說明進行測試並解讀測試結果

Regularly perform the test and interpret result according to IFU

使用兼容的血糖試紙並注意其使用期限

Use compatible blood glucose test strips and beware of their expiry date

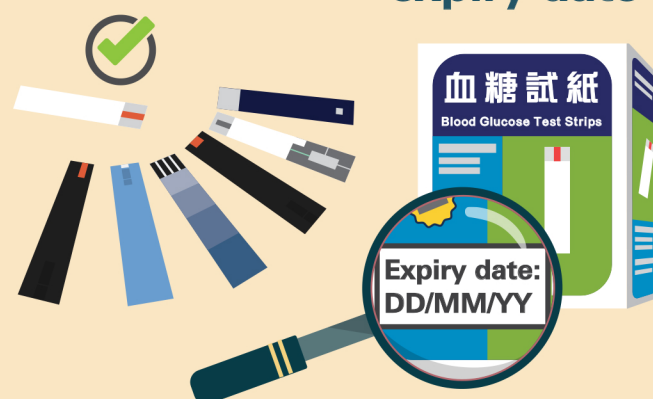

按使用說明儲存及保養器械

Store and maintain the devices according to IFU



如有病徵，請諮詢醫護人員

Consult healthcare professional if having a symptom



*已表列的醫療器械在安全、品質及性能方面均符合表列制度的要求。

Listed devices meet the listing requirements on safety, quality and performance.

更多資訊 For more information:



有關已表列的家用血糖機：
For listed home-use blood glucose meter:
<https://www.mdd.gov.hk/tc/mdacs/search-database/thematic-md/index.html>



醫療器械科
Medical Device Division
www.mdd.gov.hk



衛生署
Department of Health

二零二三年二月製作
Produced in February 2023